



TANBead® Nucleic Acid Extraction Kit

OptiPure cfDNA Auto Plate

(For use with the Maelstrom 9600 series)



W61CA46

(For Professional Use Only) V5

1. Intended Purpose

The TANBead® Nucleic Acid Extraction Kit is a nucleic acid purification kit based on magnetic bead technology by using with corresponding TANBead® Nucleic Acid Extractor, which can automatically isolate and purify cell-free DNA (cfDNA) from human serum and plasma. The purified cfDNA can be used with any downstream application employing PCR-based qualitative, semi-quantitative, quantitative assays and capillary electrophoresis. The kit is intended for use by technicians, physicians, and biologists with well-trained in molecular biological techniques, the techniques of magnetic bead purification and *in vitro* diagnostic procedures. Any diagnostic results generated by using the sample preparation procedure in conjunction with any downstream diagnostic assay should be interpreted related to other clinical or laboratory findings. The kit is not limited to any specific disorder, condition, or other additional accompanying diagnostics. It is applicable for all population.

2. The basic principle

The silicon dioxide layer coated on the magnetic beads can adsorb the negatively charged molecules to purify nucleic acids from samples.

3. Specification

Starting Materials	500~1000 µL plasma / serum
Elution Volume	70~100 µL
Typical DNA yield	1~100 ng per mL plasma / serum
Typical DNA size	100~300 bp

△ DNA yield will vary from 1~100 ng according to sample source and storage method. The average DNA yield is 20 ng per mL of serum from healthy individuals.

4. Component Supplied with the Kit

Auto Plate	7	Auto Plate with reagent buffers
Proteinase K	1.0 mL x 4	Proteinase K
Elution Buffer	1.5 mL x 1	Nuclease-Free Water
Protocol	1	Instruction guide for user
Spin tips	96 tips	Spin tip assembled box

5. Auto Plate Content and Plate Position

Plate position	Buffer	Volume (µL)
1	Lysis Buffer	800
2	Lysis Buffer	800
3	Washing Buffer 1	1000
4	Washing Buffer 2	1000
5	Washing Buffer 2	1000
6	Magnetic Beads	500
7	Elution Buffer	100
8	Spin Tip	-

6. Kit Storage and Shelf Life

- Components under room temperature (15~35°C) can be stored until the expiration date labeled on the box.
- The proteinase K is transported at room temperature. Upon received, please store proteinase K at 2~8°C.

7. Precautions

- It can be used for *in vitro* diagnostic.
- When the temperature is below 20°C, place the reagent plate in an oven (preheated 42~60°C) from 5 to 10 minutes.
- Avoid vigorous shaking, in order to avoid excessive formation of foam.
- Carefully remove aluminum foil to avoid splashing.
- Do not expose the opened reagents or Auto Plates / Auto Tubes to air. The evaporation would lead to pH change, or effect on the extraction effectiveness.
- The reagents are all colorless and transparent. Colored reagents indicate contamination, please replace it with a fresh Auto Plates / Auto Tubes before proceeding.

- Please check the integrity of the Auto Plates / Auto Tubes and remember to mount the spin tips into the appropriate position of the suitable instrument before operating them.
- Please wear a mask and disposable gloves when handling.
- Use sterile consumables to avoid nuclease contamination.
- Reagent solution contains guanidine salt, avoid using bleach containing detergent.
- Avoid eyes, skin, and clothing contact with reagents. In case of any contact, flush with flowing water.
- If any serious incident occurs, please report to the manufacturer and the competent authority of the member state in which the user and / or the patient is established.

8. Materials required, Not Supplied

- TANBead® Nucleic Acid Extraction System
Model: Maelstrom 9600 series (non-sterile)
- Disposable gloves
- Scissors, utility knives
- Micropipette, disposable tips (10 µL / 200 µL / 1000 µL)
- 1.5 mL microcentrifuge tube
- 15 mL / 50 mL conical tube
- 20% SDS (Sodium dodecyl sulfate)
- Streck Cell-Free DNA BCT tubes or other Cell-Free DNA collection tube

9. Sample Collection, Storage and Transportation

■ Sample collection and storage

- Prepare cell-free plasma sample
 - Blood samples collected in Streck Cell-Free DNA BCT tubes is recommended. It is stable for up to 14 days.
 - Centrifuge whole blood at **1600 x g** for **10 minutes**.
 - Transfer the upper plasma layer to a new conical tube.
 - Centrifuge at **16000 x g** for **10 minutes**.
 - Carefully transfer the supernatant to a new conical tube for cfDNA isolation.
- Prepare cell-free serum
 - Blood samples collected in serum separator tube.
 - Let the blood clot for at least **30 minutes** in room temperature.
 - Centrifuge whole blood at **1600 x g** for **10 minutes**.
 - Transfer the upper serum layer to a new conical tube.
 - Centrifuge at **16000 x g** for **10 minutes**.
 - Carefully transfer the supernatant to a new conical tube for cfDNA isolation.
- Specimen storage
 - After centrifugation, the plasma / serum can be stored at
 - 2~8°C up to 7 days
 - 20°C for long-term preservation

■ Specimen transportation

Transportation of whole blood, plasma and serum specimens should be followed by specific pathogen transportation-related regulations. The whole blood sample should be kept between 2~25°C during transportation and within 6 hours for separated serum. Plasma / Serum sample can be transported between 2~8°C or by frozen.

10. Nucleic Acids Extraction Protocol

- Add the following components to a microcentrifuge tube:

Sample volume	Proteinase K	20% SDS
500 µL	20 µL	30 µL
1000 µL	40 µL	60 µL

- Mix well and incubate at **60°C** for **20 minutes**.
- Carefully remove the aluminum foil on the Auto Plates.
- Add sample into Auto Plate as described in below table.

Sample volume	Plate 1	Plate 2
500 µL	500 µL	N / A
1000 µL	500 µL	500 µL

- 5) Select the program "61C". The parameters are given in following section.
- 6) Follow the guide shown on the screen and place plates carefully. Make sure that the chamfer of the plate faces toward the same direction.
- 7) Carefully remove the Auto Plates when the program is finished.
- 8) Use micropipette to transfer the purified nucleic acids from **plate #7** to a clean tube.
- 9) Discard used Auto Plates and spin tips into the waste recycling bin.

11. Program

■ Maelstrom 9600 series

Program Name: 61C								
Plate	1	2	3	4	5	6	7	8
Volume (μL)	1300	1300	1000	1000	1000	500	100	-
Keep Temp.	0	0	0	-	-	0	-	-
Action	For.	For.	For.	For.	For.	For.	For.	-
Name	LB	WB1	MB	WB2	WB2	EB	-	TIP
Step	Plate	Temp. (°C)	Mixing (min)	Mixing (rpm)	Collect (sec)	Vapor (min)	Pause	
1	6	0	0.5	1000	30	0	Off	
2	1	0	10	1000	60	0	Off	
3	2	0	10	1000	60	0	Off	
4	3	0	10	1000	60	0	Off	
5	4	-	2	1500	30	0	Off	
6	5	-	2	1500	30	10	Off	
7	7	-	8	1500	60	0	Off	
8	6	0	0.2	1500	0	0	Off	

⚠ Temperature set as "0" represents room temperature!


■ Maelstrom 9610 series

Program Name: 61C								
Plate	1	2	3	4	5	6	7	8
Volume (μL)	1300	1300	1000	1000	1000	500	100	-
Keep Temp.	25	25	25	-	-	25	-	-
Action	For.	For.	For.	For.	For.	For.	For.	-
Name	LB	WB1	MB	WB2	WB2	EB	-	TIP
Step	Plate	Temp. (°C)	Mixing (min)	Mixing (rpm)	Collect (sec)	Vapor (min)	Pause	
1	6	25	0.5	1000	30	0	Off	
2	1	25	10	1000	60	0	Off	
3	2	25	10	1000	60	0	Off	
4	3	25	10	1000	60	0	Off	
5	4	-	2	1500	30	0	Off	
6	5	-	2	1500	30	10	Off	
7	7	-	8	1500	60	0	Off	
8	6	25	0.2	1500	0	0	Off	

⚠ Temperature set as "25" represents room temperature!

12. Result

Total DNA yield was quantified using Qubit dsDNA HS assay kit: 1~100 ng per mL serum / plasma. The expected peak bp (100~300 bp fragments) and low amount of gDNA contamination were observed by using Qsep 100 capillary gel electrophoresis system. The cfDNA isolate from 0.5 mL / 1.0 mL serum was shown in red / black line.

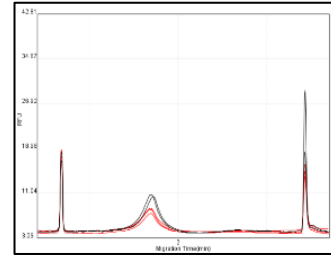

13. Reagent performance

■ Repeatability

Under repeatability conditions where nucleic acids are extracted with the same reagent kit on the same source samples by the same operator. The coefficient of variation of nucleic acid extraction concentration is less than 5%.

■ Reproducibility

A five-day reproducibility test was carried out with the same source samples for 5 consecutive days with the same reagent kit by different operators. The coefficient of variation of nucleic acid extraction concentration is less than 5%.

■ The stability of extracted DNA

Storage Conditions	DNA stability
-80°C	Over 90 days
-20°C	28 days
4°C	14 days
25°C	2 days
Freeze-thaw	5 times

14. Explanation of Symbols

	Manufacturer		Consult instructions for use
	Temperature limit		Contains sufficient for test
	CE mark		In vitro diagnostic medical use
	Catalogue number		Caution
	Batch code		Non-sterile
	Do not re-use		Keep away from sunlight
	Date of manufacture		Use-by date

EC REP

mdi Europa GmbH, Langenhagener Str. 71, 30855 Langenhagen, Germany

15. Post-market surveillance conclusion

After a risk assessment and clinical evaluation assessment, when weighing the benefits of medical device, patients, and the risks associated with the use of the device, the risk is acceptable. The post-market surveillance report shows that no death or serious adverse events occurred.